

### 1) Setting up of Bluetooth connection

In the case of your PC not having Bluetooth built in, insert a Bluetooth dongle (contained in your pump kit) to a USB port of your PC or laptop.

Please refer to the Bluetooth user manual for detailed information of any Bluetooth device.

### 2) Connection setting between PC and DANA insulin pump with Bluetooth


Connect PC and DANA insulin pump. This procedure is required at once for each following cases.

- At the first time of communication with the PC.
- In the case that the previous communication information in the PC was deleted.

#### 1. Connection Process

A. Execute 'Bluetooth Unit' and go to "Control Panel" in your PC. Find the Bluetooth icon and double click it.

B. Add 'Bluetooth Unit'

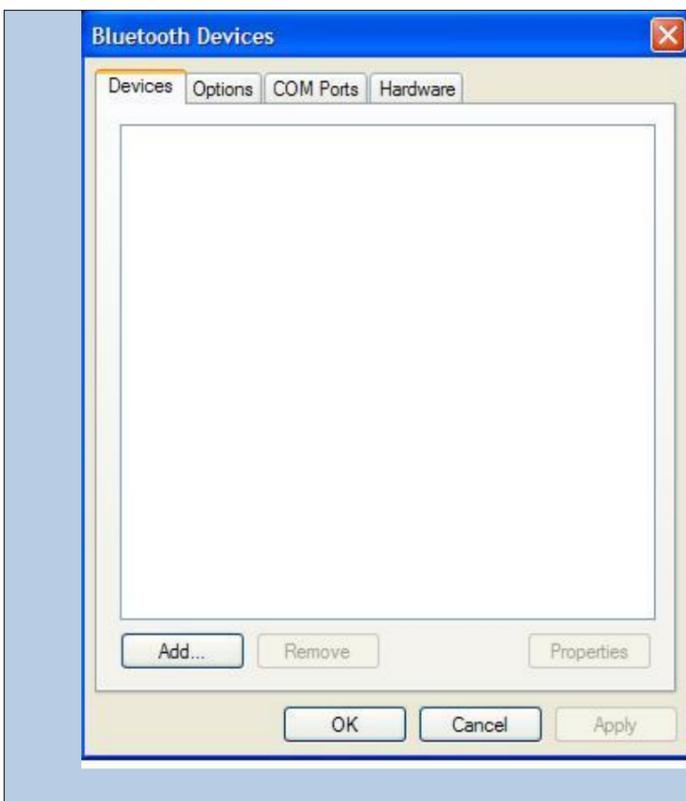

Click 'Add' to add a new Bluetooth device to your list of connected Bluetooth devices.

C. Set Discovery mode of DANA insulin pump



(figure 1)

This is the procedure to keep the DANA pump waiting for communication with a bluetooth receiver.

a. In the MAIN MENU screen press **N** until the SETTING icon is highlighted. Then press **S**. (figure 1)



(figure 2)



(figure 3)

b. The SETTING MENU screen will appear. Use **N** to highlight the DISCOVERY icon and press **S** (figure 2)

c.  Discovery Icon blinks for 60 seconds (figure3)


d. Screen will be changed to initial display once changes saved.

#### D. Initiate the Add Bluetooth Device Wizard




Tick on 'Unit set and ready to search' and click 'Next' button.

#### E. Search Unit

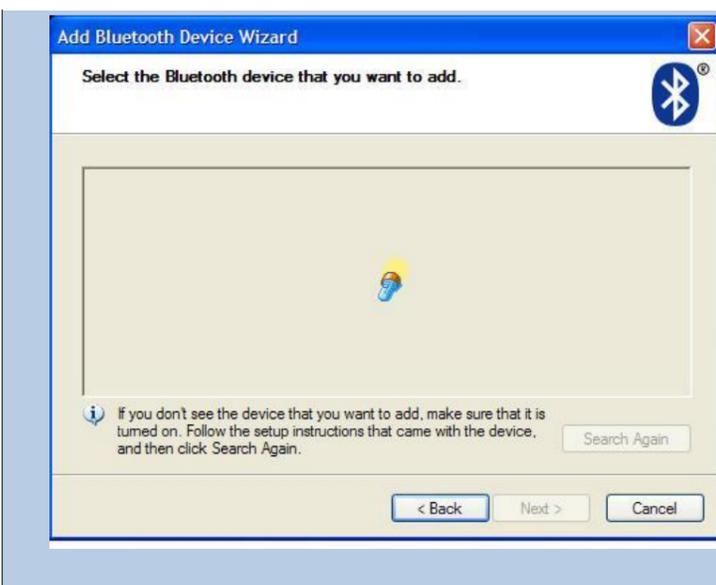


Searching bluetooth takes about 10 -15 seconds.

F. Select Bluetooth Unit

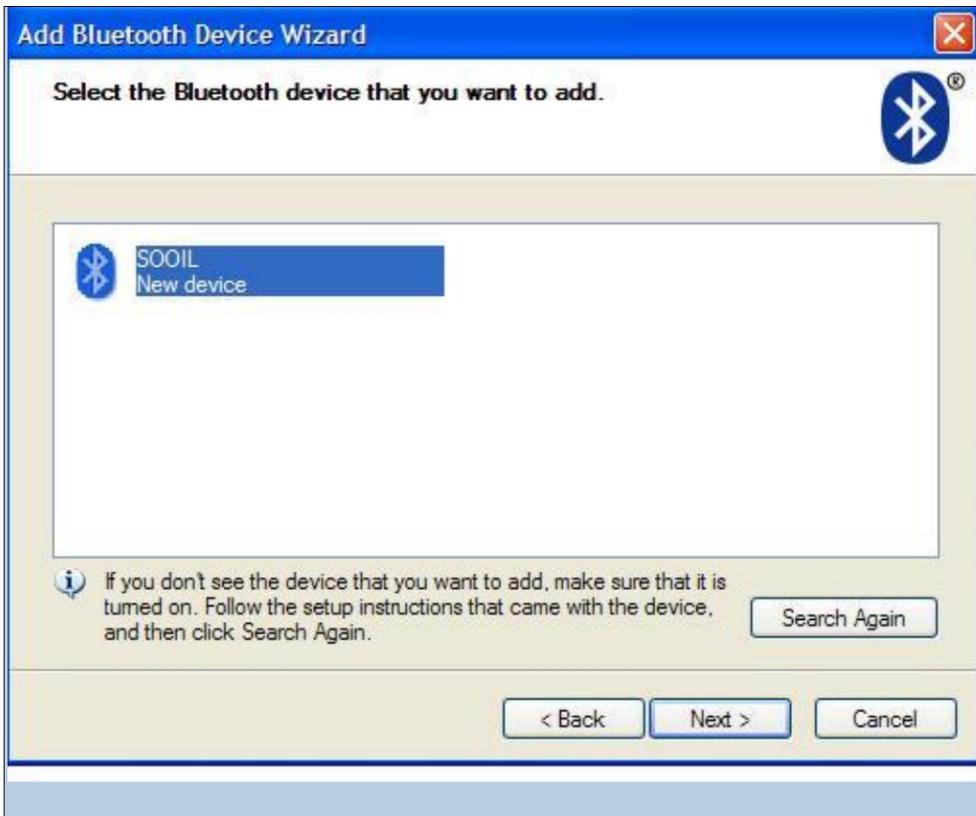

Insulin pump will be listed as a serial number.  
Add unit and click "NEXT" to continue.  
\* In case the device is not found, check your insulin pump for whether it is in discovery mode.  
- Please note: Insulin pump and remote control must not be connected each other.

G. PIN code Set up

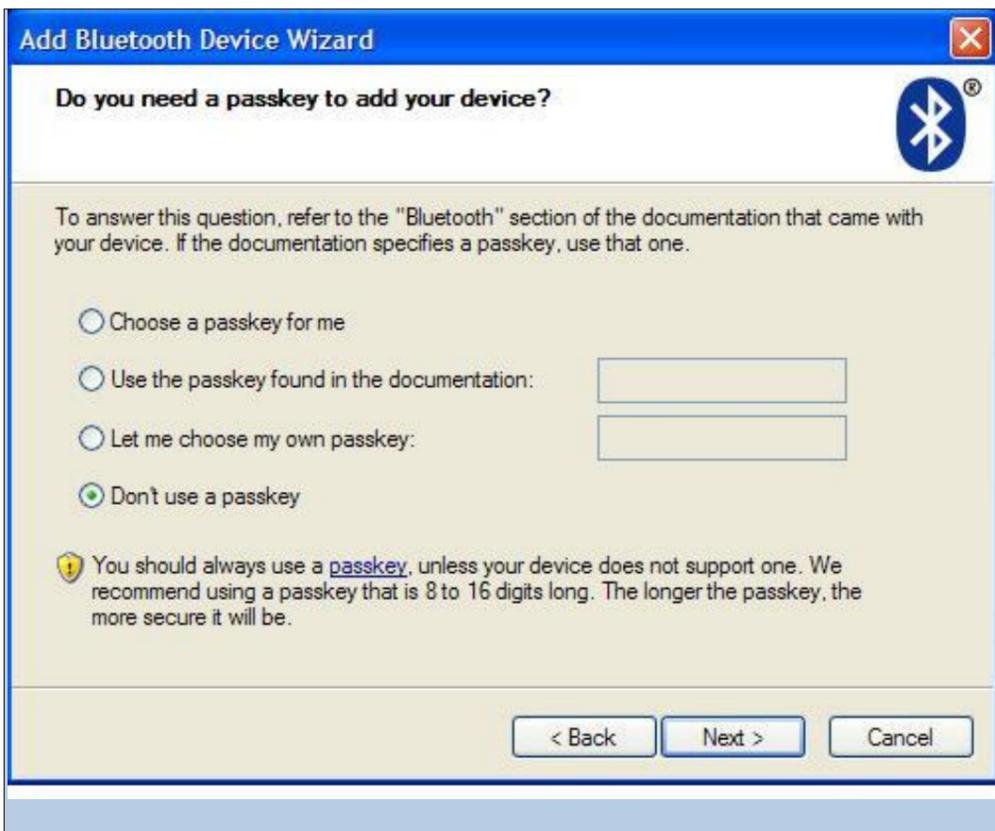


Select 'directly select PIN code'  
Set the PIN code as '0000'.  
\* In case 'no PIN code use' is selected, this browser will be displayed again. The PIN code must be set.

H. Complete Adding Bluetooth Unit




Add bluetooth unit completed.  
**Memorise the outgoing COM port name.**  
Click 'Done' to finish.

[Note] COM Port Check

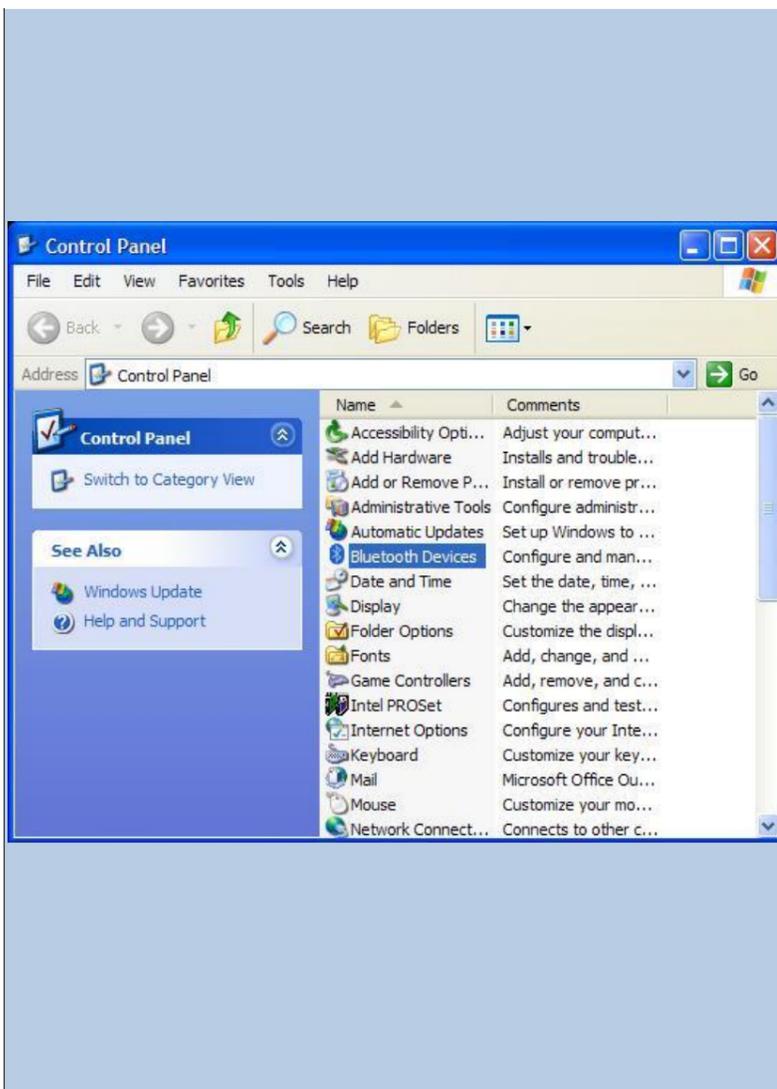


Doublecheck COM port name.  
In case the com port was not memorised, double click bluetooth unit in the Control Panel to check the outgoing COM port.

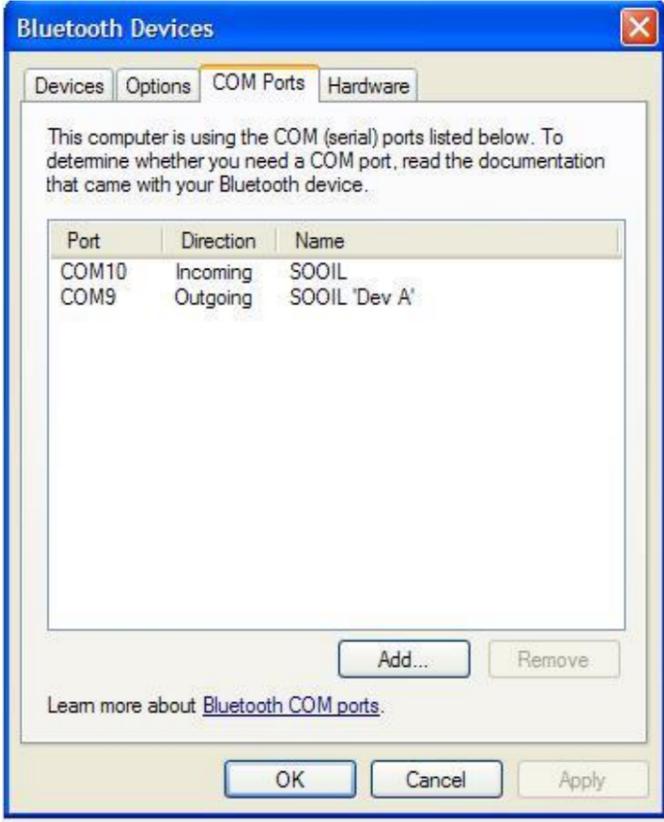


## Connecting IME-DC Dana Diabecare R via Bluetooth


I. To read out the pump in SiDiary, click on the 5th button from the left in the toolbar:

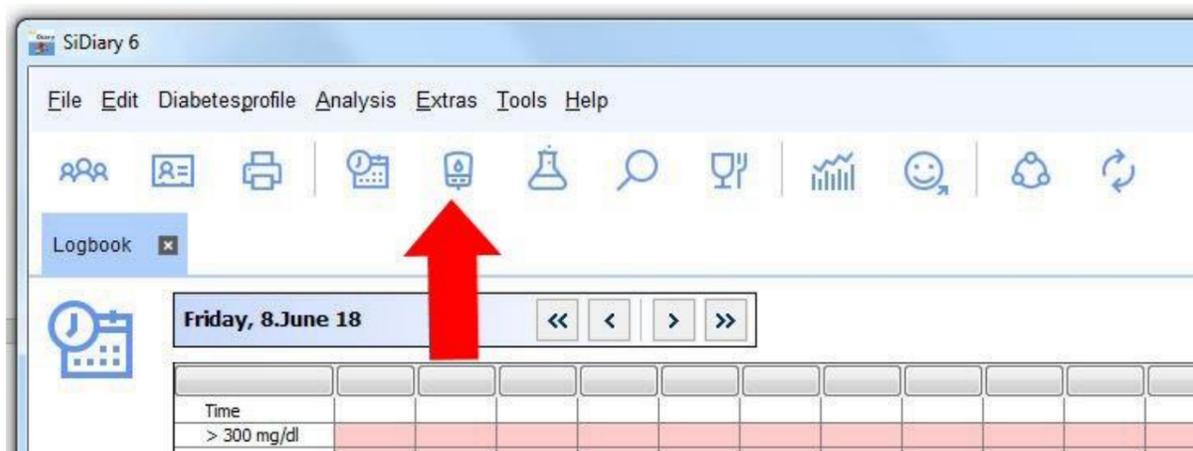

J. Select "IME-DC Dana Diabecare R" from the list of devices :

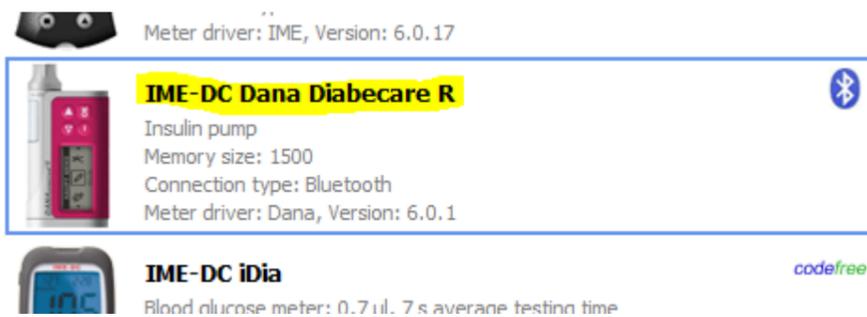

K. In the "Other COM port" field, enter the number of the outgoing COM port that you determined in step H:

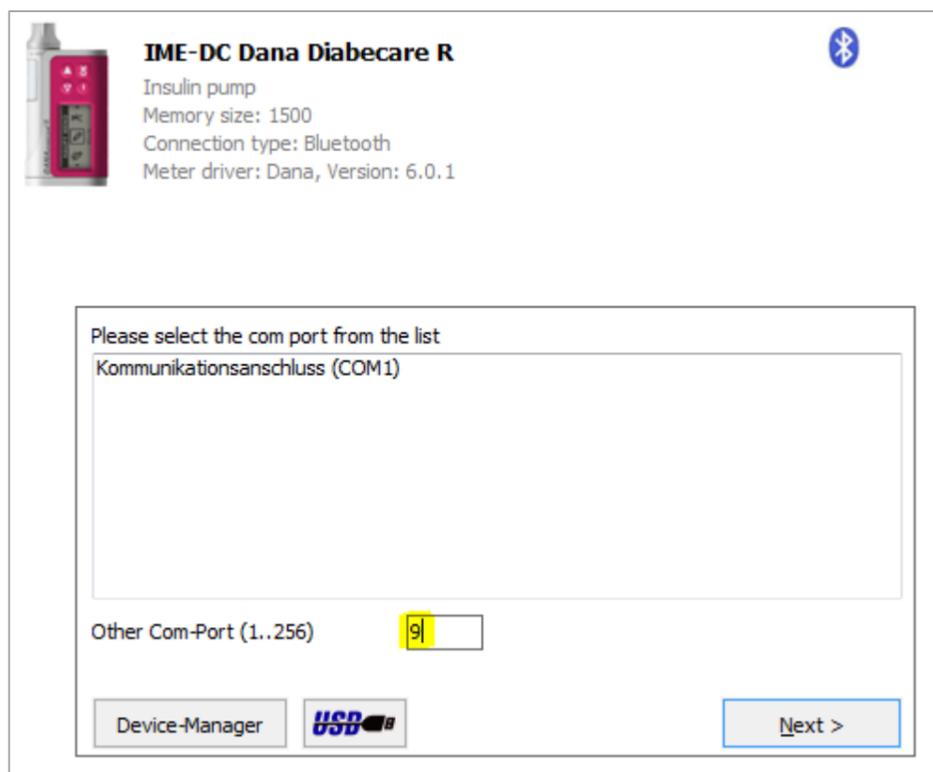

L. Then click on "Next" to start the data transfer.